



# **SARS-CoV-2 Mutation Detection HV 69-70 Deletion**

SARS-CoV-2 Mutation Detection HV 69-70 Deletion Assay is an isothermal RT-LAMP laboratory research use assays for detection of spike gene mutation HV 69-70 Deletion found in the **SARS-CoV-2 lineage B.1.1.7**

Cat. no.: X-KIT-101

V01-04-2021

**LABORATORY RESEARCH USE ONLY**

## **CONTENTS**

	Page
1 Intended Use	2
2 Summary and Test Principle	2
3 Safety Notes	2
4 Materials	3
5 Technical Data	3
6 LOOP Amplification Procedure	3
6.1 Instrumentation/Materials Required	3
6.2 Sample Collection/Preparation	3
6.3 Reagent Preparation / Storage	3
6.4 Technical Notes	3
6.5 Assay Procedure	3
6.6 Interpretation of results	4
8 Flowchart	4
9 Literature	4

## 1 INTENDED USE

SARS-CoV-2 Mutation Detection – HV 69-70 Deletion assay is an isothermal RT-LAMP laboratory research use assay for detection of spike gene mutation HV 69-70 Deletion found in the SARS-CoV-2 lineage B.1.1.7

Genetic variants of SARS-CoV-2 RNA can be found in the liquid from upper or lower respiratory tracts of infected individuals. Samples can be obtained from isolated viral RNA from naso- or oropharyngeal, swabs. Infection with any variant of SARS-CoV-2 can occur without showing any symptoms.

Negative RT-LAMP results do not exclude present or hinder future infection with SARS-CoV-2 virus or any genetic variations and the result should always be combined with clinical observations, patient history, and epidemiological information.

SARS-CoV-2 Variant Detection Assays are intended for use by science and health professionals or qualified laboratory personnel specifically instructed and trained in molecular testing techniques as well as proficient in handling biological samples.

## 2 SUMMARY AND TEST PRINCIPLE

There is an urgent need for high throughput and rapid detection of SARS-CoV-2 infections and identification of variants of concern. To address this challenge, BioThinx has developed a new line of research use RT-LAMP assay systems which can detect marker mutations found in SARS-CoV-2 variants of concern: cluster B.1.1.7, cluster B.1.351, cluster P.1. An additional assay is intended for SARS-CoV-2 general detection without mutation differentiation. All assays come in an easy to handle high-throughput format.

Molecular testing uses one-step reverse transcription and loop-mediated isothermal amplification (RT-LAMP) method.

The primers of this LAMP assay have been designed to target marker mutation **HV 69/70 deletion** within the spike protein gene found in SARS-CoV-2 lineage **B.1.1.7** (British Variant).

Initially in the United Kingdom (UK), a new variant of SARS-CoV-2 emerged with a large number of mutations. This variant has since been detected in numerous countries around the world and is associated with increased transmissibility. Beside other mutations, the UK SARS-CoV-2 lineage B.1.1.7 has multiple mutations in the spike glycoprotein's gene S. Five are amino acid replacements (D614G, A222V, N439K, Y453F and N501Y), and one deletion (HV 69-70).

## 3 SAFETY NOTES

This product is for LABORATORY RESEARCH USE ONLY, not for diagnostic, therapeutic, drug, household, or other uses. Please consult the Material Safety Data Sheet for information regarding hazards and safe handling practices.

This test kit should be handled only by qualified personnel trained in laboratory procedures and familiar with their potential hazards. Wear appropriate protective clothing, gloves and eye/face protection and handle appropriately with the requisite Good Laboratory Practices.

Treat all biological specimens, including used assay tubes and transfer pipettes, as if capable of transmitting infectious agents

Follow your institution's safety procedures for working with chemicals and handling biological samples.

Wear laboratory coats, laboratory gloves and eye protection when handling biological samples and reagents.

Remove gloves and wash hands thoroughly after handling samples and reagents.

Do not open the tubes or unseal wells during or after amplification.

Dispose of all specimens and material used to perform the test as though they contain an infectious agent. Laboratory, chemical or biohazardous wastes must be handled and discarded in accordance with all local, state and federal regulations for hazardous material.

## 4 MATERIALS

Loop amplification reaction tubes. 5 strips  
 Clear PCR single Cap 8-tube strips 200 µl;  
 optical clear flat cap; high profile; cut able;  
 filled with dried stabilized loop  
 amplification and detection mix.

LAMP reaction buffer 1 vial, 1000 µl

Negative Control 1 vial, 50 µl

Positive Control 1 vial, 50 µl

## 5 TECHNICAL DATA

Sample: purified RNA  
 Sample volume: 2 µl  
 Total incubation: 45 min at 65 °C  
 Sensitivity: < 500 targets/µl  
 Shipment: ambient temperature  
 Storage: -20 °C  
 Shelf life: 12 months after  
 manufacturing or  
 until the expiration  
 date  
 Package size: 40 tests

## 6 LOOP AMPLIFICATION PROCEDURE

### 6.1 INSTRUMENTATION AND MATERIALS REQUIRED

- PCR instrument or incubator programmable at 65 °C constant temperature
- Pipettes for 1-20 µl
- Pipette tips with aerosol filters
- Collection Kits:  
 Nasopharyngeal Swab  
 Nasal Swab
- Extraction Kit:  
 Viral DNA/RNA Extraction Kit

### 6.2 SAMPLE COLLECTION / PREPARATION

Preferentially, use the same RNA sample from which SARS-CoV-2 was detected, to genotype it for mutations. Ineffective or inappropriate sample collection can result in false test results. Extracted RNA should always be stored at -70°C or lower in an RNase free environment.

### 6.3 REAGENT PREPARATION / STORAGE

The SARS-COV-2 Mutation Detection Assay is stabilized and shipped at ambient temperature. Reagents must be stored at -20 °C upon arrival.

The reaction tubes are prefilled with LAMP reaction mixture and are supplied in a convenient dry stabilized format, containing all buffer reagents, primers, dNTPs and enzymes to perform the amplification and detection.

LAMP reaction buffer, positive and negative control are liquid and ready to use.

When stored refrigerated at -20 °C the components are stable for at least 30 days after opening or until the expiration date printed on the labels. Remaining reaction tubes should be stored refrigerated at -20 °C protected from moisture; store together with desiccant in the resealable bag (ZipLoc).

### 6.4 TECHNICAL NOTES

External control RNA should routinely be assayed as unknowns to check performance of the reagents and the assay.

Use disposable filter tips to dispense reaction buffer and samples. To avoid carryover contamination, change the tip between each sample.

### 6.5 ASSAY PROCEDURE

Strictly follow the procedure and Good Laboratory Practice.

Please adhere strictly to the sequence of pipetting steps provided in this protocol. Observe the guidelines for performing quality control in medical laboratories by assaying external controls.

All reagents should be stored refrigerated at -20 °C in their original container.

Do not exchange kit components from different lots. The expiration dates stated on the labels of the shipping container and all vials have to be observed. Do not use kit components after their expiration dates.

Reagents removed from refrigerator should be brought to room temperature. Prepare a sufficient number of microtubes to accommodate samples and controls.


1. Pipette **20 µl** of LAMP reaction buffer into the tubes.
2. Incubate for 5 minutes at room temperature (18 - 28°C).
3. For each test vial add **2 µl** sample (isolated RNA) or positive- or negative controls.
4. Close reaction tubes
5. Mix until dried reagent mixture is completely dissolved
6. Incubate for **45 min at 65 °C**.
7. Cool for 5 minutes at room temperature
8. Evaluate samples, the positive control must be blue-green and the negative control pink. Read individual samples according the negative and positive control.

## 6.6 INTERPRETATION OF RESULTS

Possible results of the different SARS-COV-2 Detection Assays:

Marker	British Lineage B.1.1.7	South African B.1.351	Brazilian P1	SARS-COV2 Hu-1
<b>N501Y</b>	+	+	+	-
<b>HV69/70 Deletion</b>	+	-	-	-
<b>E484K</b>	-	+	+	-
<b>K417T</b>	-	-	+	-
<b>E1/O117 gene</b>	+	+	+	+

## 7 FLOWCHART

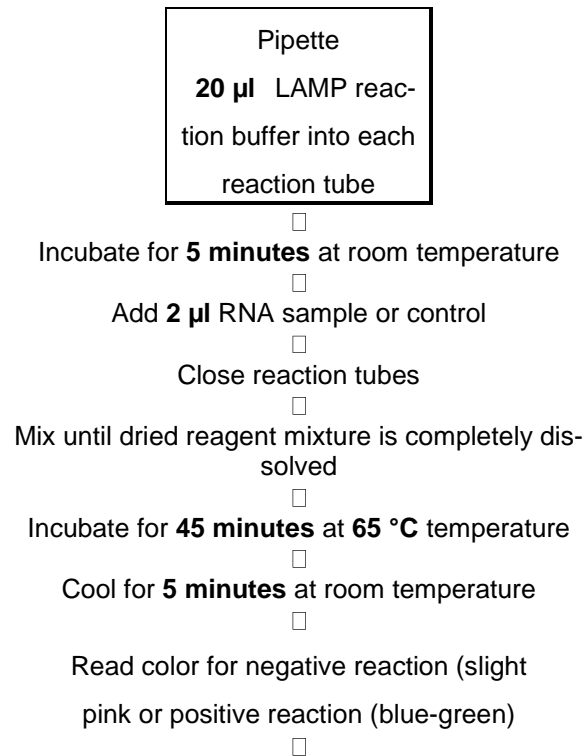

## 8 LITERATURE

WHO. 2020. Coronavirus disease 2019. World Health Organization, Geneva, Switzerland. <https://www.who.int/emergencies/diseases/novel-coronavirus-2019>.

Lu R, et al., Genomic characterisation and epidemiology of 2019 novel coronavirus: implications for virus origins and receptor binding. *Lancet* 395:565–574. (2020)

Notomi T., et al: Loop-mediated isothermal amplification of DNA, *Nucleic Acids Research*, 28(12), e63, 2000.

Mori Y., et al: Detection of loop-mediated isothermal amplification reaction by turbidity derived from magnesium pyrophosphate formation, *Biochem. Biophys. Res. Commun.*, 289(1), 150-154, 2001.

Tomita N., et al: Loop-mediated isothermal amplification (LAMP) of gene sequences and simple visual detection of products, *Nat Protoc.*, 3(5), 877-882, 2008

### **BioThinX GmbH & Co. KG**

Carl-Zeiss-Straße 51  
55129 Mainz - Germany